

Metallic materials — Rockwell hardness test —

**Part 2: Verification and calibration of
testing machines (scales A, B, C, D, E, F,
G, H, K, N, T)**

The European Standard EN ISO 6508-2:2005 has the status of a
British Standard

ICS 77.040.10

National foreword

This British Standard is the official English language version of EN ISO 6508-2:2005. It is identical with ISO 6508-2:2005. It supersedes BS EN ISO 6508-2:1999 which is withdrawn.

The UK participation in its preparation was entrusted by Technical Committee ISE/NFE/4, Mechanical testing of metals, to Subcommittee ISE/NFE/4/5, Indentation hardness testing, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this subcommittee can be obtained on request to its secretary.

Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the *BSI Catalogue* under the section entitled “International Standards Correspondence Index”, or by using the “Search” facility of the *BSI Electronic Catalogue* or of British Standards Online.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, the EN ISO title page, the EN ISO foreword page, the ISO title page, pages ii to v, a blank page, pages 1 to 18, an inside back cover and a back cover.

The BSI copyright notice displayed in this document indicates when the document was last issued.

Amendments issued since publication

Amd. No.	Date	Comments

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 10 January 2006

© BSI 10 January 2006

English Version

**Metallic materials - Rockwell hardness test - Part 2: Verification
and calibration of testing machines (scales A, B, C, D, E, F, G,
H, K, N, T) (ISO 6508-2:2005)**

Matériaux métalliques - Essai de dureté Rockwell - Partie 2:
Vérification et étalonnage des machines d'essai (échelles
A, B, C, D, E, F, G, H, K, N, T) (ISO 6508-2:2005)

Metallische Werkstoffe - Härteprüfung nach Rockwell - Teil
2: Prüfung und Kalibrierung der Prüfmaschinen (Skalen A,
B, C, D, E, F, G, H, K, N, T) (ISO 6508-2:2005)

This European Standard was approved by CEN on 14 December 2005.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

Foreword

This document (EN ISO 6508-2:2005) has been prepared by Technical Committee ISO/TC 164 "Mechanical testing of metals" in collaboration with Technical Committee ECISS/TC 1 "Steel - Mechanical testing", the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by June 2006, and conflicting national standards shall be withdrawn at the latest by June 2006.

This document supersedes EN ISO 6508-2:1999.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

Endorsement notice

The text of ISO 6508-2:2005 has been approved by CEN as EN ISO 6508-2:2005 without any modifications.

INTERNATIONAL
STANDARD

ISO
6508-2

Second edition
2005-12-15

**Metallic materials — Rockwell hardness
test —**

Part 2:

**Verification and calibration of testing
machines (scales A, B, C, D, E, F, G, H, K,
N, T)**

Matériaux métalliques — Essai de dureté Rockwell —

*Partie 2: Vérification et étalonnage des machines d'essai (échelles A, B,
C, D, E, F, G, H, K, N, T)*



Contents

Page

Foreword..... iv

Introduction v

1 Scope 1

2 Normative references 1

3 General conditions 1

4 Direct verification..... 2

5 Indirect verification..... 5

6 Intervals between verifications 8

7 Verification report/calibration certificate 8

Annex A (normative) Repeatability of testing machines..... 9

Annex B (informative) Uncertainty of measurement of the calibration results of the hardness testing machine..... 11

Bibliography 18

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 6508-2 was prepared by Technical Committee ISO/TC 164, *Mechanical testing of metals*, Subcommittee SC 3, *Hardness testing*.

This second edition cancels and replaces the first edition (ISO 6508-2:1999), which has been technically revised.

ISO 6508 consists of the following parts, under the general title *Metallic materials — Rockwell hardness test*:

- *Part 1: Test method (scales A, B, C, D, E, F, G, H, K, N, T)*
- *Part 2: Verification and calibration of testing machines (scales A, B, C, D, E, F, G, H, K, N, T)*
- *Part 3: Calibration of reference blocks (scales A, B, C, D, E, F, G, H, K, N, T)*

Introduction

Attention is drawn to the fact that, in this part of ISO 6508, the use of hardmetal for ball indenters is considered to be the standard type of Rockwell indenter ball. Steel indenter balls may be continued to be used if specified in a product specification, or by special agreement.

10/10/2020 10:10:10 AM

Metallic materials — Rockwell hardness test —

Part 2:

Verification and calibration of testing machines (scales A, B, C, D, E, F, G, H, K, N, T)

1 Scope

This part of ISO 6508 specifies a method of verification of testing machines for determining Rockwell hardness (scales A, B, C, D, E, F, G, H, K, N, T) in accordance with ISO 6508-1.

It specifies a direct method for checking the main functions of the machine operation and an indirect method suitable for the overall checking of the machine. The indirect method may be used on its own for periodic routine checking of the machine in service.

If a testing machine is also to be used for other methods of hardness testing, it shall be verified independently for each method.

This part of ISO 6508 is applicable to portable hardness testing machines.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 376:2004, *Metallic materials — Calibration of force-proving instruments used for verification of uniaxial testing machines*

ISO 6507-1, *Metallic materials — Vickers hardness test — Part 1: Test method*

ISO 6508-1, *Metallic materials — Rockwell hardness test — Part 1: Test method (scales A, B, C, D, E, F, G, H, K, N, T)*

ISO 6508-3:2005, *Metallic materials — Rockwell hardness test — Part 3: Calibration of reference blocks (scales A, B, C, D, E, F, G, H, K, N, T)*

3 General conditions

Before a Rockwell hardness testing machine is verified, the machine shall be checked to ensure that it is properly set up in accordance with the manufacturer's instructions:

Especially it should be checked that:

- a) the plunger holding the indenter is capable of sliding in its guide;

- b) the indenter-holder is firmly mounted in the plunger;
- c) the test force can be applied and removed without shock or vibration and in such a manner that the readings are not influenced.

It shall be checked that the readings are not affected either by movements of the test piece or by deformation of the frame. When a device is supplied, which locks the test piece against the upper part of the frame, the locking force shall exceed the total test force. The influence of deformations may be checked by using a plunger with a spherical tip (diameter of at least 10 mm), instead of the indenter, bearing against the anvil through a spacer and using the locking device when it is supplied. The material of the plunger and of the spacer have a hardness of at least 60 HRC. The readings of the measuring system (with preliminary force applied) before application and after removal of the additional force shall not differ by more than 1,5 Rockwell units (without locking equipment) and 0,5 Rockwell units (with locking equipment).

4 Direct verification

4.1 General

4.1.1 Direct verification should be carried out at a temperature of $(23 \pm 5) ^\circ\text{C}$. If the verification is made outside of this temperature range, this shall be reported in the verification report.

4.1.2 The instruments used for verification and calibration shall be traceable to national standards.

4.1.3 Direct verification involves:

- a) calibration of the test force;
- b) verification of the indenter;
- c) calibration of the depth-measuring system;
- d) verification of the testing cycle.

4.2 Calibration of the test force

4.2.1 The preliminary test force F_0 (see 4.2.4) and each total test force F used (see 4.2.5) shall be measured, and, whenever applicable, this shall be done at not less than three positions of the plunger spaced throughout its range of movement during testing. The preliminary test force shall be held for at least 2 s.

4.2.2 Three readings shall be taken for each force at each position of the plunger. Immediately before each reading is taken, the plunger shall be moved in the same direction as during testing.

4.2.3 The forces shall be measured by one of the following two methods:

- by means of a force proving device in accordance with ISO 376:2004, class 1, or
- by balancing against a force, accurate to $\pm 0,2 \%$, applied by means of calibrated masses or by another method having the same accuracy.

4.2.4 The tolerance on the preliminary test force F_0 (before application and after removal of the additional test force F_1) shall be $\pm 2,0 \%$.

4.2.5 The tolerance on the total test force F shall be $\pm 1,0 \%$. Each individual value of F shall be within this tolerance.

4.3 Verification of the indenter

4.3.1 Diamond cone indenter (scales A, C, D, N)

To verify the reliable performance of the conical indenter in conformance with this part of ISO 6508, a direct and an indirect verification shall be carried out.

4.3.1.1 Direct verification

4.3.1.1.1 The surfaces of the diamond cone and spherical tip shall be polished for a penetration depth of 0,3 mm and shall blend in a truly tangential manner. Both surfaces shall be free from surface defects.

4.3.1.1.2 The verification of the shape of the indenter can be made by direct measurement or by measurement of its projection on a screen. The verification shall be made at not less than four equally spaced sections.

4.3.1.1.3 The diamond cone shall have an included angle of $(120 \pm 0,35)^\circ$.

Deviations from straightness of the generatrix of the diamond cone, adjacent to the blend, shall not exceed 0,002 mm over a minimum length of 0,4 mm.

4.3.1.1.4 The angle between the axis of the diamond cone and the axis of the indenter-holder (normal to the seating surface) shall not exceed $0,5^\circ$.

4.3.1.1.5 The tip of the indenter shall be spherical. Its radius shall be determined from single values, measured in the axial section planes defined in 4.3.1.1.2. The distance between the concentric circles shall be no more than 0,004 mm. Each single value shall be within $(0,2 \pm 0,015)$ mm. The mean value out of at least four single values shall be within $(0,2 \pm 0,01)$ mm.

NOTE 1 The radius can be obtained by determining the intersection of two segments of the concentric circles.

NOTE 2 The single value is the mean value of the two radii of the concentric circles.

Measurement with a collimator device is also available. In this case, the measurements should be carried out at least in four central angles and the central angle of 120° must be included.

4.3.1.2 Indirect verification

The hardness values given by the testing machine depend not only on the dimensions given in 4.3.1.1.3 and 4.3.1.1.5, but also on the surface roughness and the position of the crystallographic axes of the diamond, and the seating of the diamond in its holder.

To examine this influence, the indirect verification of the indenter shall be performed on four reference blocks which shall be calibrated for the hardness levels given in Table 1 or on blocks giving equivalent total depths of indentation.

Table 1 — Hardness levels for different scales

Scale	Hardness	Ranges
HRC	23	20 to 26
HRC	55	52 to 58
HR45N	43	40 to 46
HR15N	91	88 to 94

EN ISO 6508-2:2005

For each block, the mean hardness value of three indentations made using the indenter to be verified shall not differ from the mean hardness value of the three indentations obtained with the indenter, calibrated in accordance with 4.5 of ISO 6508-3:2005 by more than $\pm 0,8$ Rockwell units. The indentations made with the indenter to be verified and with the above-mentioned indenter should be adjacent.

NOTE This can be performed with a calibration machine in accordance with the procedure described in Clause 5 of ISO 6508-3:2005.

The hardness testing machines used for this indirect verification shall comply with the following tolerances for the test forces:

$$F_0: \pm 1,0 \%$$

$$F: \pm 0,5 \%$$

The test shall be carried out in accordance with ISO 6508-1.

4.3.2 Ball indenter (scales B, E, F, G, H, K, T)

4.3.2.1 For the purpose of verifying the size and the hardness of the balls, one sample selected at random from a batch shall be tested. The balls verified for hardness shall be discarded.

4.3.2.2 The balls shall be polished and free from surface defects.

4.3.2.3 The user shall either measure the balls to ensure that they meet the following requirements, or shall obtain balls from a supplier certifying that the following conditions are met.

4.3.2.3.1 The diameter, measured at no less than three positions, shall not differ from the nominal diameter by more than the tolerance given in Table 2.

Table 2 — Tolerances for the different ball diameters

Rockwell hardness scale	Ball diameter mm	Tolerance mm
B	1,587 5	$\pm 0,003 5$
F	1,587 5	$\pm 0,003 5$
G	1,587 5	$\pm 0,003 5$
T	1,587 5	$\pm 0,003 5$
E	3,175	$\pm 0,004$
H	3,175	$\pm 0,004$
K	3,175	$\pm 0,004$

4.3.2.3.2 The characteristics of the hardmetal balls shall be as follows:

— hardness: the hardness shall be no less than 1 500 HV, when determined using a test force of at least 4,903 N in accordance with ISO 6507-1. The hardmetal ball may be tested directly on this spherical surface or by sectioning the ball and testing on the ball interior. An example for HV 10 is given in Table 3.

— density: $\rho = (14,8 \pm 0,2) \text{ g/cm}^3$.

NOTE The following chemical composition is recommended:

- tungsten carbide (WC) balance
- total other carbides 2,0 %
- cobalt (Co) 5,0 % to 7,0 %

4.3.2.3.3 The hardness of steel balls shall be no less than 750 HV, when determined using a test force of 98,07 N in accordance with ISO 6507-1 (see Table 3).

Table 3 — Values of the mean diagonal (HV10) for the determination of the hardness of the ball indenters

Ball diameter mm	Maximum value of the mean diagonal made on the spherical surface of the ball with a Vickers indenter at 98,07 N (HV10) mm	
	Steel ball	Hardmetal ball
3,175	0,153	0,109
1,587 5	0,150	0,107

4.4 Calibration of the depth-measuring system

4.4.1 The depth-measuring system shall be calibrated over no less than three intervals, including the intervals corresponding to the lowest and highest hardness for which the scales are normally used, by making known incremental movements of the indenter in the direction of increasing hardness values.

4.4.2 The instrument used to verify the depth-measuring system shall have an accuracy of 0,000 2 mm. The depth-measuring system shall correctly indicate within $\pm 0,001$ mm for the scales A to K and within $\pm 0,000 5$ mm for scales N and T, i. e. within $\pm 0,5$ of a scale unit, over each range.

NOTE If it is not possible to verify the depth-measuring system directly, its performance can be derived from the results of an indirect verification, using reference blocks and a certified indenter, and making corrections for known errors (see 5.2).

4.5 Verification of the testing cycle

The testing cycle shall conform to the testing cycle given in ISO 6508-1 and shall be timed with an uncertainty less than $\pm 0,5$ s.

5 Indirect verification

5.1 General

Indirect verification should be carried out at a temperature of (23 ± 5) °C by means of reference blocks calibrated in accordance with ISO 6508-3. If the verification is made outside of this temperature range, this shall be reported in the verification report.

5.2 Procedure

5.2.1 For the indirect verification of a testing machine, the following procedures shall be applied.

The testing machine shall be verified for each scale for which it shall be used. For each scale to be verified, reference blocks from each of the hardness ranges given in Table 4 shall be used. The hardness values of the blocks shall be chosen to approximate the limits of the intended use.

5.2.2 On each reference block, five indentations shall be uniformly distributed over the test surface and each hardness number observed to within 0,2 of a scale unit. Before making these indentations, at least two preliminary indentations shall be made to ensure that the machine is working freely and that the reference block, the indenter and the anvil are seating correctly. The results of these preliminary indentations shall be ignored. The test shall be made in accordance with ISO 6508-1.

Table 4 — Hardness ranges for different scales

Rockwell hardness scale	Hardness range of reference block	Rockwell hardness scale	Hardness range of reference block
A	20 to 40 HRA 45 to 75 HRA 80 to 88 HRA	K	40 to 60 HRK 65 to 80 HRK 85 to 100 HRK
B	20 to 50 HRB 60 to 80 HRB 85 to 100 HRB	15N	70 to 77 HR15N 78 to 88 HR15N 89 to 91 HR15N
C	20 to 30 HRC 35 to 55 HRC 60 to 70 HRC	30N	42 to 54 HR30N 55 to 73 HR30N 74 to 80 HR30N
D	40 to 47 HRD 55 to 63 HRD 70 to 77 HRD	45N	20 to 31 HR45N 32 to 61 HR45N 63 to 70 HR45N
E	70 to 77 HRE 84 to 90 HRE 93 to 100 HRE	15T	73 to 80 HR15T 81 to 87 HR15T 88 to 93 HR15T
F	60 to 75 HRF 80 to 90 HRF 94 to 100 HRF	30T	43 to 56 HR30T 57 to 69 HR30T 70 to 82 HR30T
G	30 to 50 HRG 55 to 75 HRG 80 to 94 HRG	45T	12 to 33 HR45T 34 to 54 HR45T 55 to 72 HR45T
H	80 to 94 HRH 96 to 100 HRH		

5.3 Repeatability

5.3.1 For each reference block, let H_1, H_2, H_3, H_4, H_5 be the values of the measured hardness arranged in increasing order of magnitude.

The repeatability r of the testing machine, under the particular verification conditions, is determined by the following quantity:

$$r = H_5 - H_1 \quad (1)$$

The mean hardness value of the five indentations \bar{H} is defined as follows:

$$\bar{H} = \frac{H_1 + H_2 + H_3 + H_4 + H_5}{5} \quad (2)$$

where H_1, H_2, H_3, H_4, H_5 are the hardness values corresponding to the five indentations.

5.3.2 The repeatability of the testing machine being verified shall be considered satisfactory if it satisfies the conditions given in Table 5. Permissible repeatability is presented graphically in Figures A.1 and A.2.

Table 5 — Permissible repeatability and error of the testing machine

Rockwell hardness scale	Hardness range of the reference block	Permissible error Rockwell units	Permissible repeatability of the testing machine ^a
A	20 to ≤ 75 HRA > 75 to ≤ 88 HRA	± 2 HRA ± 1,5 HRA	≤ 0,02 (100 - \bar{H}) or 0,8 Rockwell units ^b
B	20 to ≤ 45 HRB > 45 to ≤ 80 HRB > 80 to ≤ 100 HRB	± 4 HRB ± 3 HRB ± 2 HRB	≤ 0,04 (130 - \bar{H}) or 1,2 Rockwell units ^b
C	20 to ≤ 70 HRC	± 1,5 HRC	≤ 0,02 (100 - \bar{H}) or 0,8 Rockwell units ^b
D	40 to ≤ 70 HRD > 70 to ≤ 77 HRD	± 2 HRD ± 1,5 HRD	≤ 0,02 (100 - \bar{H}) or 0,8 Rockwell units ^b
E	70 to ≤ 90 HRE > 90 to ≤ 100 HRE	± 2,5 HRE ± 2 HRE	≤ 0,04 (130 - \bar{H}) or 1,2 Rockwell units ^b
F	60 to ≤ 90 HRF > 90 to ≤ 100 HRF	± 3 HRF ± 2 HRF	≤ 0,04 (130 - \bar{H}) or 1,2 Rockwell units ^b
G	30 to ≤ 50 HRG > 50 to ≤ 75 HRG > 75 to ≤ 94 HRG	± 6 HRG ± 4,5 HRG ± 3 HRG	≤ 0,04 (130 - \bar{H}) or 1,2 Rockwell units ^b
H	80 to ≤ 100 HRH	± 2 HRH	≤ 0,04 (130 - \bar{H}) or 1,2 Rockwell units ^b
K	40 to ≤ 60 HRK > 60 to ≤ 80 HRK > 80 to ≤ 100 HRK	± 4 HRK ± 3 HRK ± 2 HRK	≤ 0,04 (130 - \bar{H}) or 1,2 Rockwell units ^b
N		± 2 HRN	≤ 0,04 (100 - \bar{H}) or 1,2 Rockwell units ^b
T		± 3 HRT	≤ 0,06 (100 - \bar{H}) or 2,4 Rockwell units ^b
^a where \bar{H} is the mean hardness value ^b whichever is greater			

5.4 Error

5.4.1 The error, E , of the testing machine under the particular verification conditions is expressed by the following equation:

$$E = \bar{H} - H_c \quad (3)$$

where

\bar{H} is the mean hardness value;

H_c is the specified hardness of the reference block used.

5.4.2 The error of the testing machine shall not exceed the values given in Table 5.

5.5 Uncertainty of measurement

The determination of the uncertainty of measurement of the calibration results of the hardness testing machines is given in Annex B.

6 Intervals between verifications

The specifications for the direct verifications of hardness testing machines are given in Table 6.

Indirect verification shall be performed at least once every 12 months and after a direct verification has been performed.

Table 6 — Direct verifications of hardness testing machines

Requirements of verification	Force	Measuring system	Test cycle	Indenter ^a
before setting to work first time	x	x	x	x
after dismantling and reassembling, if force, measuring system or test cycle are affected	x	x	x	
failure of indirect verification ^b	x	x	x	
indirect verification > 14 month ago	x	x	x	

^a In addition, it is recommended that the indenter be directly verified after 2 years of use.

^b Direct verification of these parameters may be carried out sequentially (until the machine passes indirect verification) and is not required if it can be demonstrated (e.g. by tests with a reference indenter) that the indenter was the cause of the failure.

7 Verification report/calibration certificate


The verification report/calibration certificate shall include the following information:

- a) a reference to this part of ISO 6508;
- b) method of verification (direct and/or indirect);
- c) identification data for the hardness testing machine;
- d) means of verification (reference blocks, elastic proving devices, etc.);
- e) Rockwell hardness scale(s) verified;
- f) verification temperature;
- g) result obtained;
- h) date of verification and reference to the verification institution;
- i) uncertainty of the verification result.

Annex A
(normative)

Repeatability of testing machines


The permissible repeatability of testing machines is presented graphically in Figures A.1 and A.2.

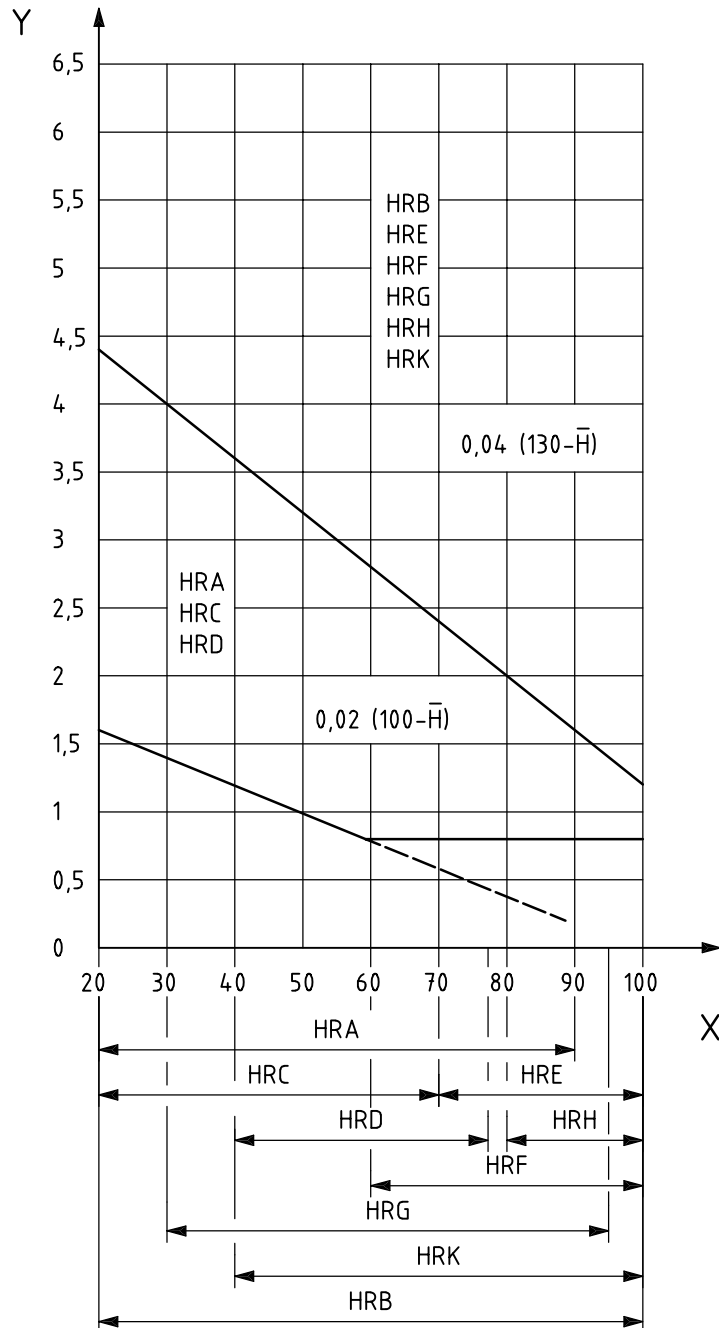

Key

- X Rockwell hardness
- Y repeatability of testing machines

Figure A.1 — Rockwell hardness (scales A, B, C, D, E, F, G, H and K)

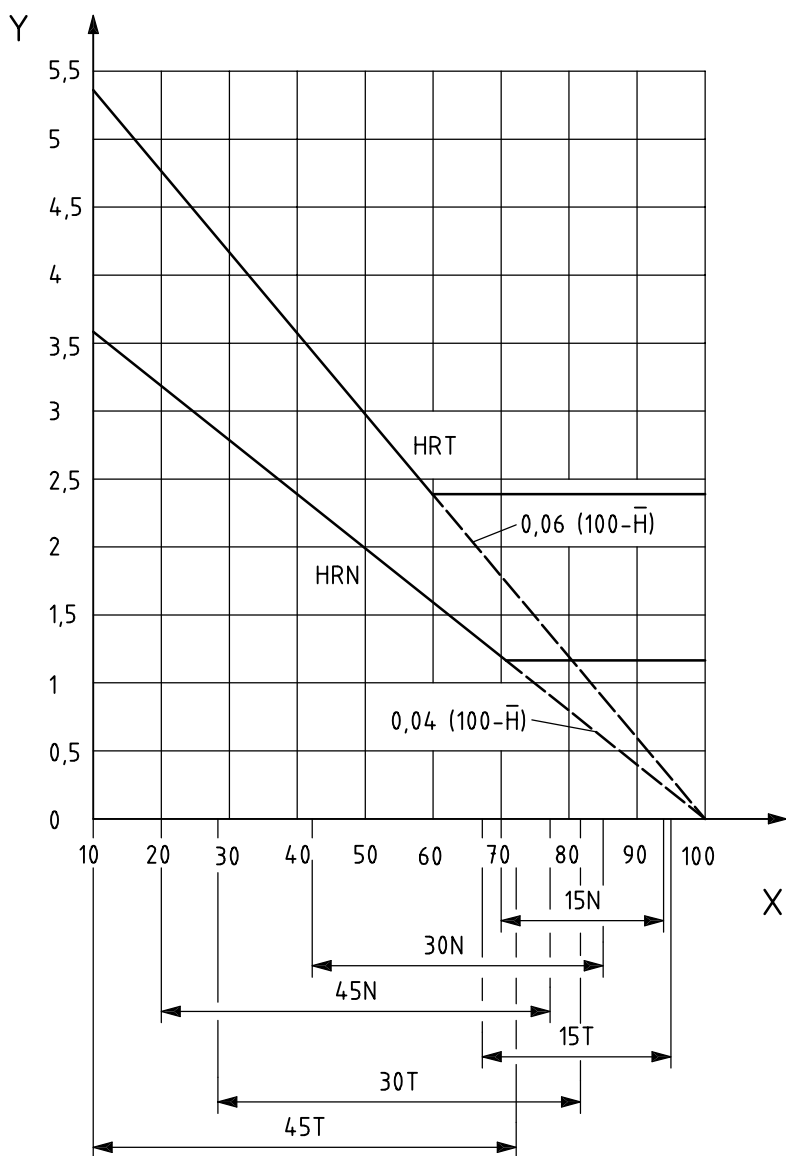

Key

- X Rockwell hardness
- Y repeatability of testing machines

Figure A.2 — Rockwell superficial hardness (scales N and T)

Annex B (informative)

Uncertainty of measurement of the calibration results of the hardness testing machine

B.1 Direct calibration of the hardness testing machine

B.1.1 Calibration of the test force

The combined relative standard uncertainty of the test force calibration is calculated according to the following equation:

$$u_F = \sqrt{u_{FRS}^2 + u_{FHTM}^2} \quad (\text{B.1})$$

with

u_{FRS} is the relative uncertainty of measurement of the force transducer (from calibration certificate);

u_{FHTM} is the relative standard uncertainty of the test force generated by the hardness testing machine.

The uncertainty of measurement of the reference instrument, force transducer, is indicated in the corresponding calibration certificate. The influence quantities, like

- temperature dependence,
- long-term stability, and
- interpolation deviation,

should be considered for critical applications. Depending on the design of the force transducer, the rotational position of the transducer related to the indenter axis of the hardness testing machine should be considered.

NOTE The metrological chain necessary to define and disseminate hardness scales is shown in Figure G.1 in ISO 6508-1:2005.

For example

Uncertainty of measurement of the force transducer (from calibration certificate): $U_{FRS} = 0,12 \% (k = 2)$

Calibration value of the force transducer $F_{RS} = 1471,0 \text{ N}$

Table B.1 — Results of the test force calibration

Number of height position for test force calibration	Series 1	Series 2	Series 3	Mean value	Relative deviation	Relative standard measurement uncertainty
	F_1 N	F_2 N	F_3 N	\bar{F} N	ΔF_{rel} %	u_{FHTM} %
1	1 471,5	1 471,9	1 471,7	1 471,7	0,05	0,008
2	1 472,1	1 472,3	1 472,7	1 472,3	0,09	0,012
3	1 472,2	1 473,5	1 471,3	1 472,3	0,09	0,043

where

$$\Delta F_{rel} = \frac{F_{RS} - \bar{F}}{\bar{F}} \tag{B.2}$$

$$u_{FHTM} = \frac{s_{Fi}}{F} \cdot \frac{1}{\sqrt{n}}, (n = 3) \tag{B.3}$$

s_{Fi} is the standard deviation of the test-force indication values in the i -th height position.

In Table B.2, the maximum value of u_{FHTM} from Table B.1 is used.

Table B.2 — Calculation of the uncertainty of measurement of the test force

Quantity	Estimated value	Relative limit values	Distribution type	Relative standard measurement uncertainty	Sensitivity coefficient	Relative uncertainty contribution
X_i	x_i	a_i		$u(x_i)$	c_i	$u_i(H)$
u_{FRS}	1 471,0 N		Normal	$6,0 \times 10^{-4}$	1	$6,0 \times 10^{-4}$
u_{FHTM}	1 471,0 N		Normal	$4,3 \times 10^{-4}$	1	$4,3 \times 10^{-4}$
Relative combined standard uncertainty u_F						$7,4 \times 10^{-4}$
Relative expanded uncertainty of measurement $U_F (k = 2)$						$1,5 \times 10^{-3}$

Table B.3 — Calculation of the maximum relative deviation of the test force including the uncertainty of measurement of the reference instrument

Relative deviation of test force	Expanded relative uncertainty of test force	Max. relative deviation of test force including measurement uncertainty of reference instrument
ΔF_{rel} %	U_F %	ΔF_{max} %
0,09	0,15	0,24

In Table B.3, ΔF_{\max} is calculated as follows:

$$\Delta F_{\max} = |\Delta F_{\text{rel}}| + U_F \tag{B.4}$$

The result of the example means that the deviation of the test force, including the uncertainty of measurement of the reference instrument specified in 4.2 amounting to $\pm 1,0 \%$, is complied with.

B.1.2 Depth-measuring system

The combined relative standard uncertainty of the reference instrument for the depth-measuring system is calculated as follows:

$$u_L = \sqrt{u_{\text{LRS}}^2 + u_{\text{ms}}^2 + u_{\text{LHTM}}^2} \tag{B.5}$$

where

- u_{LRS} is the relative uncertainty of measurement of the depth calibration device (reference standard) from the calibration certificate for $k = 1$;
- u_{ms} is the relative uncertainty of measurement due to the resolution of the measuring system;
- u_{LHTM} is the relative standard uncertainty of measurement of the hardness testing machine.

The uncertainty of measurement of the reference instrument for the depth-measuring system, the depth calibration device, is indicated in the corresponding calibration certificate. The influence quantities, for example

- temperature dependence,
- long-term stability, and
- interpolation deviation,

do not exert an essential influence on the uncertainty of measurement of the depth calibration device.

For example:

Uncertainty of measurement of depth calibration system: $u_{\text{LRS}} = 0,000\ 2 \text{ mm } (k = 2)$

Resolution of the depth-measuring system $\delta_{\text{ms}} = 0,5 \text{ }\mu\text{m}$

Table B.4 — Results of the calibration of the depth-measuring system

Rated value of the depth-measuring system	Series 1	Series 2	Series 3	Mean value	Relative deviation	Relative standard measurement uncertainty
L_{RS} mm	L_1 mm	L_2 mm	L_3 mm	\bar{L} mm	ΔL_{rel} %	u_{LHTM} %
0,060	0,060 3	0,060 2	0,060 0	0,060 2	0,33	0,15
0,080	0,080 5	0,080 3	0,080 2	0,080 3	0,38	0,11
0,100	0,100 7	0,100 2	0,100 3	0,100 4	0,40	0,15
0,120	0,120 3	0,120 5	0,120 1	0,120 3	0,25	0,10
0,140	0,140 5	0,140 6	0,140 3	0,140 5	0,33	0,06
0,160	0,160 6	0,160 3	0,160 2	0,160 4	0,23	0,07

In Table B.4:

$$u_{\text{LHTM}} = \frac{s_{\text{Li}}}{L} \cdot \frac{1}{\sqrt{n}}, (n = 3) \tag{B.6}$$

$$\Delta L_{\text{rel}} = \frac{\bar{L} - L_{\text{RS}}}{L_{\text{RS}}} \tag{B.7}$$

s_{Li} is the standard deviation of the length indication values for the i -th indication value of the object micrometer.

Table B.5 — Calculation of the uncertainty of measurement of the measuring system

Quantity	Estimated value	Limit value	Distribution type	Relative standard measurement uncertainty	Sensitivity coefficient	Uncertainty contribution
X_i	x_i	a_i		$u(x_i)$	c_i	$u_i(H)$
u_{LRS}	0 mm	$1,0 \times 10^{-4}$ mm	Normal	$1,0 \times 10^{-4}$	1	$1,0 \times 10^{-4}$
u_{ms}	0 mm	$0,5 \times 10^{-4}$ mm	Rectangular	$1,8 \times 10^{-4}$	1	$1,8 \times 10^{-4}$
u_{LHTM}	0,06 mm	0,15 %	Normal	$9,6 \times 10^{-4}$	1	$9,6 \times 10^{-4}$
Relative combined uncertainty of measurement u_L , (related to 0,16 mm), %						0,098
Relative expanded uncertainty of measurement U_L ($k = 2$), %						0,20

Table B.6 — Calculation of the maximum relative deviation of the measuring system including the uncertainty of measurement of the length reference instrument

Test length	Relative deviation of the measuring system	Expanded relative uncertainty of measurement	Max. relative deviation of measuring system including measurement uncertainty of length reference instrument
L_{RS} mm	ΔL_{rel} %	U_L %	ΔL_{max} %
0,16 mm	0,33	0,20	0,53

In Table B.6:

$$\Delta L_{\text{max}} = |\Delta L_{\text{rel}}| + U_L \tag{B.8}$$

The result of the example means that the deviation of the measuring system, including the uncertainty of measurement of the length reference instrument specified in 4.4 amounting to $\pm 1,0 \mu\text{m}$ ($L_{\text{RS}} \times \Delta L_{\text{max}} = 0,16 \text{ mm} \times 0,57 \% = 0,000 91 \text{ mm}$), is complied with.

B.1.3 Verification of the indenter

The indenter, consisting of indenter tip and holder, cannot be verified respectively calibrated, in-site. A valid calibration certificate of an accredited calibration laboratory shall exist which confirms the geometrical deviations of the indenter (see 4.3).

B.1.4 Verification of the test cycle

In 4.5, the permissible deviation for every section of the test cycle is stipulated as ± 0,5 s. While measuring with a usual time measuring system (stopwatch), the uncertainty of measurement can be indicated as 0,1 s. Therefore, an estimation of the uncertainty of measurement is not necessary.

B.2 Indirect verification of the hardness testing machine

NOTE In this Annex, the index “CRM (Certified Reference Material)” means, according to the definitions of the hardness testing standards, “Hardness Reference Block”.

By indirect verification with hardness reference blocks, the overall function of the hardness testing machine is checked and the repeatability, as well as the deviation of the hardness testing machine from the real hardness value, are determined.

The uncertainty of measurement of the indirect verification of the hardness testing machine follows from the equation:

$$u_{HTM} = \sqrt{u_{CRM}^2 + u_{CRM-D}^2 + u_{ms}^2} \tag{B.9}$$

where

- u_{CRM} is the calibration uncertainty of the hardness reference block according to the calibration certificate for $k = 1$;
- u_{CRM-D} is the hardness change of the hardness reference block since its last calibration due to drift (negligible for use of the hardness reference block complying with the standard);
- u_{ms} is the uncertainty due to the resolution of the hardness testing machine.

For example:

Hardness reference block	$H_{CRM} = 45,4 \text{ HRC}$
Uncertainty of measurement of the hardness reference block	$U_{CRM} = \pm 0,5 \text{ HRC}$
Resolution of the hardness testing machine	$\delta_{ms} = 0,1 \mu\text{m}$

Table B.7 — Results of the indirect verification

No.	Measured hardness value
	H, HRC^a
1	46,4 _{max}
2	46,1
3	45,3 _{min}
4	45,7
5	45,8
Mean value \bar{H}	45,9
Standard deviation s_H	0,42
^a HRC: Rockwell hardness	

In Table B.7:

$$\bar{b} = \bar{H} - H_{\text{CRM}} \tag{B.10}$$

$$\bar{b} = 45,9 - 45,4 = 0,5 \text{ HRC}$$

$$u_{\text{H}} = \frac{t \cdot s_{\text{H}}}{\sqrt{n}} \tag{B.11}$$

For $t = 1,14$, $n = 5$ and $s_{\text{H}} = 0,42$ HRC follows:

$$u_{\text{H}} = 0,21 \text{ HRC}$$

B.3 Budget of uncertainty of measurement

Table B.8 — Budget of uncertainty of measurement

Quantity	Estimated value	Standard uncertainty of measurement	Distribution type	Sensitivity coefficient	Uncertainty contribution
X_i	x_i	$u(x_i)$		c_i	$u_i(H)$
u_{CRM}	45,4 HRC	0,25 HRC	Normal	1,0	0,25 HRC
u_{ms}	0 HRC	0,029HRC	Rectangular	1,0	0,029 HRC
U_{H}	0 HRC	0,21 HRC	Normal	1,0	0,21 HRC
$u_{\text{CRM-D}}$	0 HRC	0 HRC	Triangular	1,0	0 HRC
Combined uncertainty of measurement, u_{HTM}					0,33 HRC
Expanded uncertainty of measurement, $U_{\text{HTM}} (k = 2)$					0,66 HRC
HRC: Rockwell hardness					

Table B.9 — Maximum deviation of the hardness testing machine including the uncertainty of measurement

Measured hardness on the hardness testing machine	Expanded uncertainty of measurement	Deviation of the testing machine when calibrating with the reference block	Maximum deviation of the testing machine including uncertainty of measurement
H HRC	U_{HTM} HRC	$ \bar{b} $ HRC	ΔH_{HTMmax} HRC
45,1	0,66	0,5	1,12
HRC: Rockwell hardness			

In Table B.9:

$$\Delta H_{\text{HTMmax}} = U_{\text{HTM}} + |\bar{b}| = 0,7 + 0,5 = 1,2 \text{ HRC} \tag{B.12}$$

The result of the example above means that the permissible limit deviation of the testing machine, including the uncertainty of measurement of the testing machine specified in Clause 5 amounting to $\pm 1,5$ HRC, is complied with.

Bibliography

- [1] A. SAWLA: *Uncertainty of measurement in the verification and calibration of the force measuring systems of testing machines*. Proceedings of the Asia-Pacific symposium on measurement of force, mass and torque (APMF), Tsukuba, Japan, November 2000
- [2] A. WEHRSTEDT, I. PATKOVSKY: *News in the field of standardization about verification and calibration of materials testing machines*, May 2001, EMPA Academy 2001
- [3] W. GABAUER: *Manual codes of practice for the determination of uncertainties in mechanical tests on metallic materials, The estimation of uncertainties in hardness measurements*, Project No. SMT4-CT97-2165, UNCERT COP 14:2000
- [4] T. POLZIN, D. SCHWENK: Method for Uncertainty Determination of Hardness Testing; PC File for Determination, *Materialprüfung* **44** (2002) 3, pp. 64-71

10/10/2020 10:10:10

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.

Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001.

Fax: +44 (0)20 8996 7001. Email: orders@bsi-global.com. Standards are also available from the BSI website at <http://www.bsi-global.com>.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.

Tel: +44 (0)20 8996 7111. Fax: +44 (0)20 8996 7048. Email: info@bsi-global.com.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.

Tel: +44 (0)20 8996 7002. Fax: +44 (0)20 8996 7001.

Email: membership@bsi-global.com.

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsi-global.com/bsonline>.

Further information about BSI is available on the BSI website at <http://www.bsi-global.com>.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright & Licensing Manager.

Tel: +44 (0)20 8996 7070. Fax: +44 (0)20 8996 7553.

Email: copyright@bsi-global.com.